

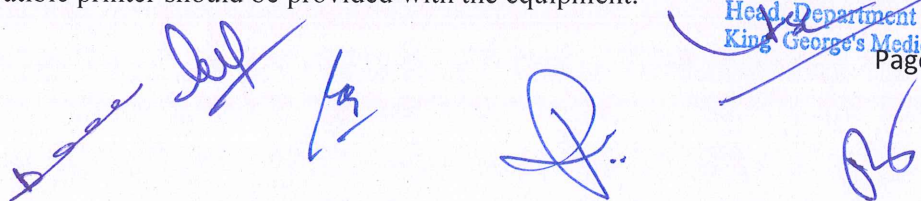
SPECIFICATIONS FOR FULLY AUTOMATED COAGULATION ANALYZER

1. Fully automated Coagulation analyzer.
2. Viscosity /Optical based detection system.
3. Should be Capable to run Clotting assay, Chromogenic assay & immunoturbidimetric assays.
4. Parameters-PT, APTT, Fibrinogen, TT, ATIII, Heparin, D-Dimer, PC, PS, FV, FVII, FVI & FIX.
5. Minimum Throughput should be 50 PT test/hour & time to first patents result – PT/APTT/FB = 8mts.
6. Should be a minimum of 80 test Methodologists available.
7. Should be a minimum of 16 Reagent positions. All should be temperature controlled & and maintained from 15 to 19 deg C. Each reagent can be placed in several positions and the analyzer will detect it automatically without manual intervention.
8. Should be Positive barcode identification for reagents. Should be Barcode identification for the reagent name, and st number. Expiry, onboard stability.
9. Should be a minimum of 20 sample carrousels for primary tubes. Capable of adapting pediatric tubes & Microtainers.
10. Should be Positive barcode identification for samples.
11. Continues sample loading with all positions for STAT node.
12. Should be at least 12 programmable tests for one sample.
13. Should be a Single probe for Samples & Reagents with LLD (Liquid level detection).
14. Should be a minimum of 200 cuvettes on board with continuous loading capability.
15. Should be Pre cerebrated assays for PT, APTT, FIB & D-Dimer.
16. Should be Storage capacity for Calibration curves. Automatic dilution for calibrations.
17. Should be multi-tasking software with a touch screen with an LCD.
18. Should be at least 600 patients' results & One-year IQC results in memory.
19. Should be QC management with Levy Jennings chart & Wesdgard QC alarms.
20. Should be the facility of Alarm for QC out range message.
21. Should be the availability of an internal printer or the capability to adapt an external printer.
22. Should be LIS capability with, BI directional transferring capacity.

Additional points for a tender document for the coagulation analyzer:-

1. Compatible printer should be provided with the equipment.

Prof. Avinash Agrawal
MD, IDCC, IFCCM, FICCM, FIACCM, FCCP (USA)
Head, Department of Critical care,
King George's Medical University, UP, Lko.
Page 1 of 4



2. Original System Packs (Reagents/consumables/controls/calibrators) for the first 500 tests each of PT & APTT shall be supplied free of cost along with the equipment.
3. All accessories, like UPS, cables, ports, spares, etc as necessary for complete, smooth, and breakdown-free functioning of the entire system shall be the responsibility of the supplier.

Conditions for tenderer:

1. All accessories should be from the same Original Equipment Manufacturer for the main unit.
2. Instruments must be ISO certified and a copy should be enclosed. (The ISO Certificate must be issued by any organization accredited by the Bureau of Indian Standard or accredited by the international accrediting forum "IAF" (Certificate to be attached).
3. Should be USA FDA and/ or European CE be approved by 4 digits notified body.
4. Other necessary certifications if any required will be provided by the bidder for the smooth functioning of the machine.
5. Installation process should be performed by O.E.M trained service engineers/ service representatives on OEM letterhead or Service Report within 15 days of supply, with the mandatory provision of providing preventive services visit of OEM trained Service Engineer/ Service Representative quarterly per year till the completion of warranty period (i.e., 20 visits for the first 05 years) & further quarterly visits (04 visits/year) year till the completion of CMC period.
6. The equipment should have a Brand name/ Model Number embossed/etched on the equipment.
7. All the technical specifications in the compliance statement must be supported by Original Literature from the firm/ O.E.M with highlighting Numbering & flagging of all technical certificates.
8. Offered Equipment should have a strong Government Installation base.
9. Offered Equipment should have a Regional Sales Service Centre of the Original Equipment Manufacturer in the region for a 95 % uptime guarantee.
10. For the offered main unit, the essential, optional required consumables'/accessories' shelf life should be declared on the Original Equipment Manufacturer's letterhead.
11. In case of technical snag/failure/breakdown the response time for the inspection should be within 24 hours and repair within 05 days otherwise provide a service

Prof. Avinash Agrawal
MD, IDCC, IFCCM, FICCM, FIACEM, FCCP (USA)
Head, Department of Critical care,
King George's Medical University, UP, Lko.

Page 2 of 4







machine/ alternate arrangement to be made till the period of recovery of the breakdown of the unit, failing which attracts penal action as per the decision of institute/ hospital.

12. For offered equipment the Training of technical staff and users should be performed by Original Equipment Manufacturer trained Service Engineers at the proper designated place- at bidders' cost.
13. Company should quote their latest model and need to provide an affidavit for the same.
14. As a tendering process the Demonstration of the offered Equipment is Mandatory at hospital/institute premises or other designated places at the bidder's cost.
15. The bidder must comply with the General Financial Rules and their modifications if any issued by the Government of India- 2017.
16. Any bidder from a country that shares a land border with India will be eligible to bid in the tender only if the bidder is registered with the Competent Authority (i.e., Registration certificate issued by the Ministry of Commerce and Industry (Department for Promotion of Industry and Internal Trade- DPIIT after October 2020). If any such bidder is not registered with DPIIT they will be liable for technical disqualification.
17. Principal (OEM) must authorize only one agent to be quoted in the bid otherwise multiple quotes through different agents in the same bid will be canceled.
18. The Bidder and its OEM both have to submit a notarized affidavit on the Indian Non-Judicial Stamp Paper of Rs.100/- that the bidder has not quoted the price higher than the current financial year and last financial year supplied to any government Institute/ Organization/ reputed Private Organization. OEM also has to submit that the price quoted by the bidder in the bid is on its behalf and the lowest in the current and last financial year in the country. Therefore, if at any stage it has been found that the supplier and its OEM have quoted lower rates than those quoted in this bid; the Institute (the purchaser) would be given the benefit of lower rates by the Supplier and any excess payment if any, will become immediately payable to the Institute (the purchaser). If such an affidavit is not submitted, the bid will be outrightly rejected. (Part of technical bid).
19. Guarantee / Warranty Period: Separate offers of Comprehensive Maintenance Contract (CMC on main equipment) and Annual Maintenance Contract (AMC on main equipment) for further 5 years after expiry of 5 years of warranty (i.e., 6th, 7th, 8th, 9th and 10th years) in rupees only (and on basis of percentage of price) should be

Dr. Vinash Agrawal
MD, IDCC, IPCCM, FICCM, FIACCM, FCCP (USA)
Head, Department of Infection Control,
King George's Medical University, UP, Lko.

included in a financial bid in the absence of which the offer is liable to be rejected. Payment for CMC/AMC shall be made only after the expiry of the warranty of 5 years, in case the Institute (the purchaser) decides for availing of CMC/AMC services. Contract for CMC/AMC shall be decided on expiry of warranty but rates (not more than 5% inclusive of all taxes for 6th to 10th year) will be frozen at the price of an issued purchase order before the release of payment by the Institute (the purchaser). However, the Institute (the purchaser) may decide not to enter into any CMC/AMC contract without assigning any reason for the same, which shall be binding upon the bid.

20. Should provide 5-year CMC. CMC cannot be more than 5% of the contract value.
21. System configured application-specific educational video tutorials shall be provided as standard with the system.
22. Details of service outlet in India to render services during 5 years warranty period.
23. The principals must give a certificate if the supplier/vendor is changed during the course of the guarantee/warranty period, the principals would be responsible for the upkeep/maintenance of the quote/supplied equipment, besides honouring all the terms and conditions of CMC/AMC in letter and spirit.

Prof. Avinash Agrawal
MD, IDCC, FCCM, FICCM, FIACCM, FCCP (USA)
Head, Department of Critical care,
King George's Medical University, UP, Lko.